

MICROTEK

Bio-5000



Medical Imaging Systems


Dry or Wet
Gel Sample



Professional Gel Scanner for
Electrophoresis Gel, SDS-PAGE, Western Blotting, etc.


Features

- 4.2 Dmax
- Designed removable waterproof glass holder
- Deliver the accurate images of gel sample
- Make batch scanning easily
- Microtek patented E.D.I.T.™

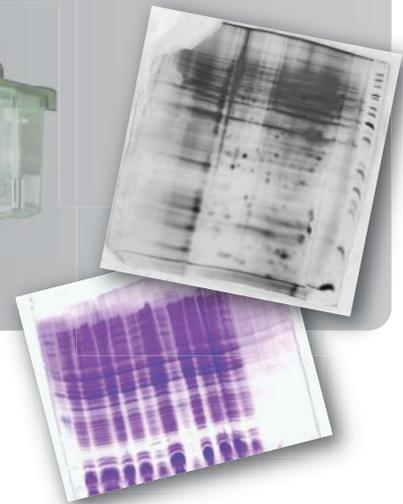

• Removable Glass Holder

Thanks to the design of Bio-5000, the glass holder can be removed anytime. The glass holders can be cleaned and washed easily. Users can capture images directly from gel surface handily no matter the samples are dry or wet.

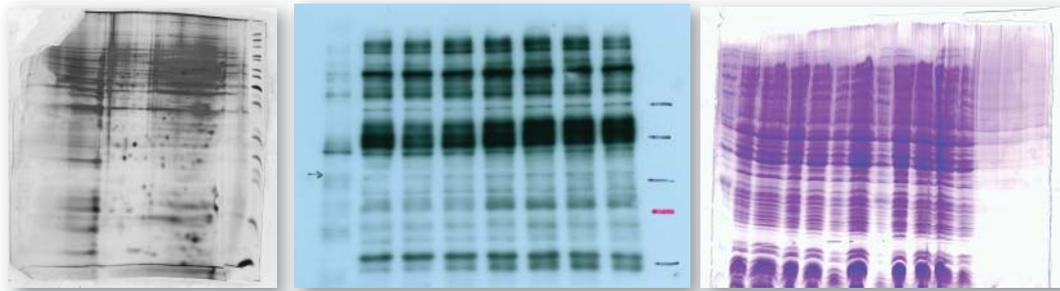

Specifications

| | |
|------------------------------|--|
| Product Type | Flatbed Scanner |
| Image Sensor | CCD |
| Scanning Area | Reflective- 8.5" x 14" / 216mm x 356mm (Legal-size) Transparent: Up to 7.7" x 9.7" / 195mm x 246mm |
| Bit Depth | True 48-bit |
| Optical Resolution | 4800 X 9600 dpi |
| Interface | Hi-Speed USB (USB 2.0) |
| Dimensions | 22.3" x 15.1" x 6.3" / 567mm x 385mm x 158mm |
| Net Weight | 28.8 lbs (13 kg) |
| Power Supply | 100 to 240 VAC, 50 to 60 Hz |
| Max Power Consumption | 35 Watts |
| Platform | Windows |
| System Requirements | * CD-ROM drive (for installing software) * Color monitor with 24-bit color capability * 128MB RAM (256MB recommended) |
| | PC and compatibles |
| | - Pentium III PC or higher with USB port - Microsoft Windows 7 / Vista / XP / 2000 |



EVESTAR GmbH
Lindtstraße 127-129
D-47877 Willich, Germany



Microtek International, Inc.
No. 6, Industry East Road 3,
Science-Based Industrial Park,
Hsinchu, 30077, Taiwan

© 2010 Microtek. Microtek, ScanWizard, the ArtixScan, and E.D.I.T. logo, are trademarks or registered trademarks of Microtek International, Inc. All other brands, product names and logos herein are trademarks or registered trademarks of their respective holders. Specifications, software bundles and accessories are subject to change without notice. Delivery of technical support services subject to change without notice. Not responsible for typographical errors. Digital Imagery © 2010 Jupiterimages Co. 012011